


Technical data sheet

OTICON | Open

CIC 75

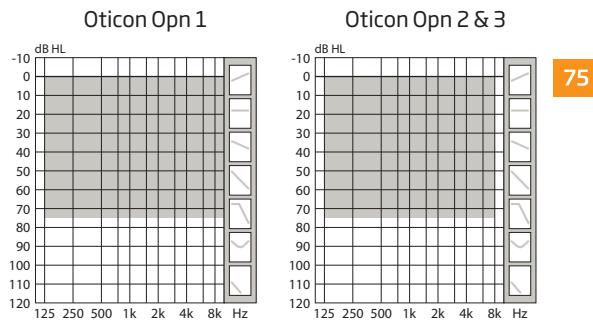

	Oticon Open 1	Oticon Open 2	Oticon Open 3	
Speech Understanding	OpenSound Navigator™	Level 1	Level 2	Level 3
	Max. noise removal	9 dB	5 dB	3 dB
	Speech Guard™ LX	Level 1	Level 2	Level 3
Sound Quality	Spatial Sound™ LX***	4 estimators (o)	2 estimators (o)	2 estimators (o)
	Soft Speech Booster LX	•	•	•
	Speech Rescue™ LX	•	•	•
	Clear Dynamics	•	•	-
	Spatial Noise Management****	o	o	-
	Fitting Bandwidth*	10 KHz	8 KHz	8 KHz
	Processing Channels	64	48	48
Listening Comfort	Transient Noise Management	4 configurations	On/Off	On/Off
	Feedback shield LX	•	•	•
	Binaural Coordination*****	o	o	o
	YouMatic™ LX	3 configurations	2 configurations	1 configuration
Personalization & Optimizing Fitting	Fitting Bands	16	14	12
	Adaptation Management	•	•	•
	Oticon Firmware Updater	•	•	•
	Fitting Formulas	VAC+, NAL-NL1+2, DSL v5.0	VAC+, NAL-NL1+2, DSL v5.0	VAC+, NAL-NL1+2, DSL v5.0
	Acoustic Notifications	•	•	•
	Tinnitus SoundSupport™*****	o	o	o
	Battery life, hours**	70-80	70-80	70-80

* Bandwidth accessible for gain adjustments during fitting

** Battery size 10 - IEC PR70.

Real usage battery life is shown as an estimated interval based on mixed use cases with variable amplification settings and variable input levels.

*** If NFMI is chosen

**** If NFMI and push button is chosen

- Default
- Optional
- Not included

OpenSound Navigator™ continuously analyzes the environment and attenuates the disturbing noise.

NFMI wireless technology is optional and provides binaural communication

Oticon Open is built on the Velox™ platform, providing frequency resolution in 64 channels (Open 1).

Fully programmable with updatable firmware, the Velox platform is ready for the future.



IP68

Call
Absolute Hearing Solutions
For Hearing Aid Deals
614-452-4280
www.absolutehearingsolutions.com


oticon
PEOPLE FIRST

Technical data		Ear Simulator			2CC Coupler		
Measured according to		IEC 60118-0:1983/AMD1:1994, IEC 60118-0:2015, IEC 60118-1:1995+AMD1:1998 CSV and IEC 60318-4:2010			ANSI S3.22-2014, IEC 60118-0:2015 and IEC 60318-5:2006		
Oticon Opn CIC 75		Opn 1	Opn 2	Opn 3	Opn 1	Opn 2	Opn 3
Frequency range Hz		100-9500	100-7500	100-7500	100-7000	100-7000	100-7000
OSPL90	Peak		119 dB SPL			109 dB SPL	
	1600 Hz		110 dB SPL			103 dB SPL	
	HFA-OSPL90		110 dB SPL			104 dB SPL	
Full-on gain*	Peak		57 dB			47 dB	
	1600 Hz		49 dB			42 dB	
	HFA-FOG		49 dB			42 dB	
Reference test gain			36 dB			27 dB	
Telecoil output (1600 Hz)	1 mA/m field		-			-	
	10 mA/m field		-			-	
	SPLITS L/R		-			-	
Total harmonic distortion (Input 70 dB SPL)	500 Hz		2 %			< 2 %	
	800 Hz		2 %			< 2 %	
	1600 Hz		3 %			2 %	
Equivalent input noise level	Omni		20 dB SPL			19 dB SPL	
Battery consumption**	Typical		1.0 mA			1.0 mA	
	Quiescent		1.0 mA			1.0 mA	
Battery life, calculated, hours***			100			100	
IRIL (IEC 60118-13:2016)			700/1400/2000 MHz: 18/12/11 dB SPL				

* Measured with the gain control of the hearing aid set to its full-on position minus 20 dB and with an input SPL of 70 dB. This is to obtain a gain response equal to the full-on gain response from e.g. IEC 60118-0+A1:1994 but without influence of feedback.

** Battery current is measured according to IEC 60118-0:1983/AMD1:1994 §7.11, IEC 60118-0:2015 §7.7 and ANSI S3.22:2014 §6.13 after a settling time of minimum 3 minutes.

*** Based on the standardised battery consumption measurement (IEC 60118-0:1983/AMD1:1994). The actual battery life depends on battery quality, use pattern, active feature set, hearing loss and sound environment.

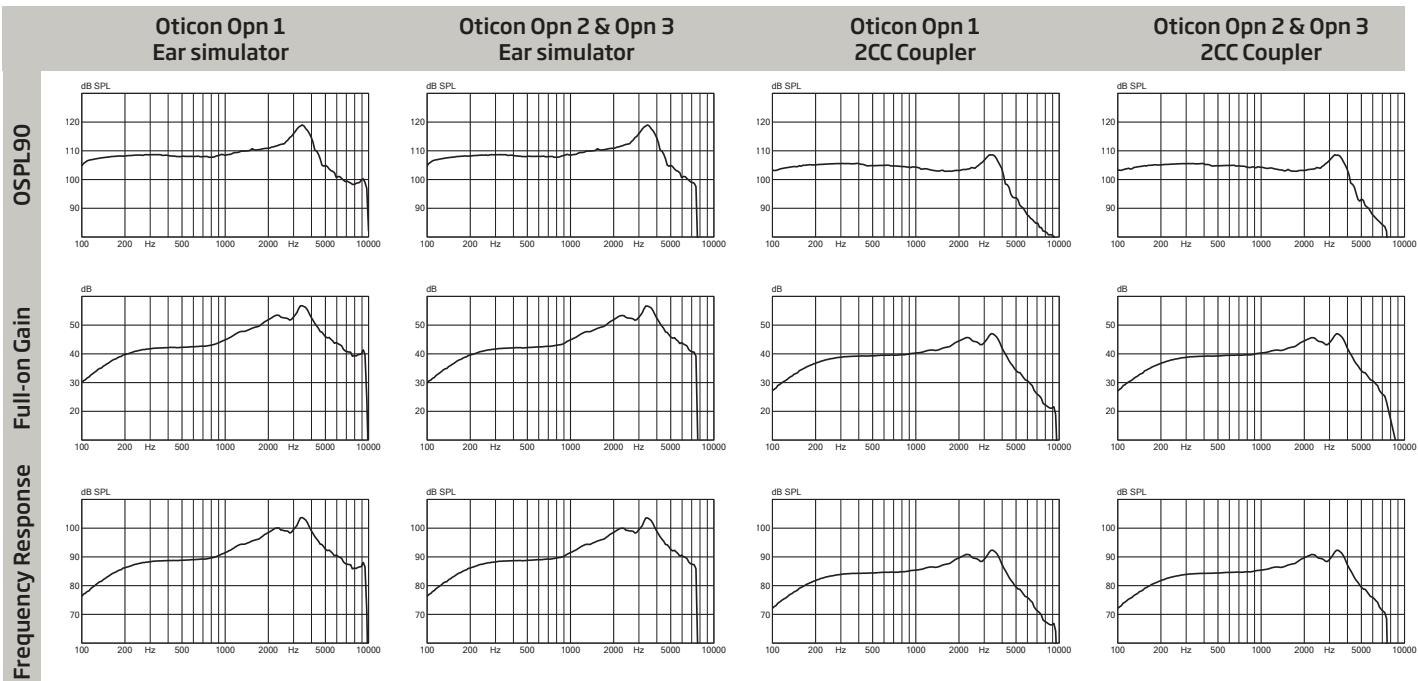

Technical information: Omnidirectional mode is used unless otherwise stated.

Operating conditions Temperature: +1°C to +40°C	Storage and transportation conditions Temperature and humidity should not exceed the following limits for extended periods during transportation and storage.
Relative humidity: 5% to 93%, non-condensing	Temperature: -25°C to +60°C Relative humidity: 5% to 93%, non-condensing

Call
Absolute Hearing Solutions
For Hearing Aid Deals
614-452-4280
www.absolutesolutions.com

oticon
PEOPLE FIRST